


KRAKEN 90

Dhydra's Patented Rapid Low Temperature Dehydration (RLTD)



SPECIFICATIONS

Dehydration Rate	165-225lb/hr (75-102kg/hr) <i>*Capacity varies depending on the density and moisture of the product</i>
Cycle Time	30-50 min
Number of Chambers	3
Number of Trays (Full Chamber)	60 trays
Process Type	Continuous operation capable of running 24/7 (1 min per tray loading cycle)
Automated Cleaning Process	Clean-in-place (CIP) system is activated by a push of a button and does not require disassembly <i>*CIP suggested before changing strains</i>
Moisture Reduction	~80% wet to ~10% dry (~4% dry for extraction) <i>*Exact moisture level can be specified based on user preferences</i>
Maximum Output (RF)	Nominally rated at 90kW (30 magnetrons @ 3kW each)
Electrical Power Requirements	2 outlets: 400V 3ph+N 180A per phase 480V 3ph 75A per phase

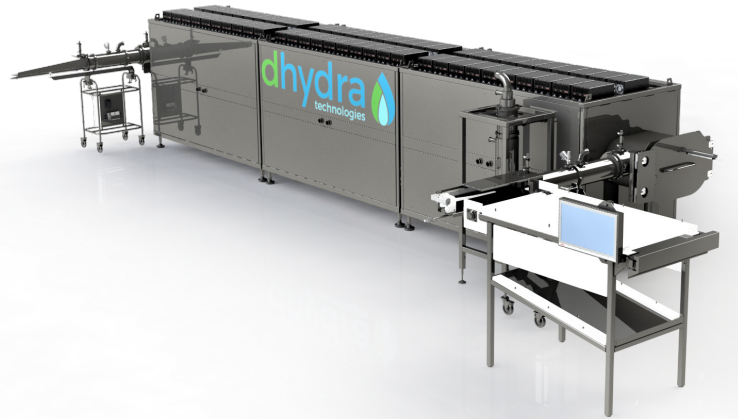

PROCESSING QUALITY

Rapid drying prevents mold proliferation
Drying in a vacuum results in virtually no oxidization
Dark conditions eliminates degradation from light
Low temperature preserves cannabinoids

- RLTD gently removes moisture in as little as 30 minutes producing a product that is shelf-stable and ready for sale
- Preserves plant integrity (e.g. fragrance, colour) using RLTD closed loop system
- Depending on the program being run, terpenes are either retained in the bud or collected in the water recovery system
- Intuitive computer control systems combined with 10,000's of sensor reading every minute, allows the machine to self-regulate and achieve uniform drying results without requiring technical staff on site
- Remote access troubleshooting services available
- Modular components for easy maintenance
- Data logins for compliance and diagnostics

CONTACT US

FILL OUT AN ONLINE FORM
TO GET STARTED

dhydra.com/contact

info@dhydratech.com | 604-566-8338

FOLLOW US FOR OUR LATEST UPDATES



@DHYDRATECH

SYSTEM REQUIREMENTS



- Drainage: floor drain
- Relative humidity (environment): dry conditions required in the packaging room; users determine humidity level
- Heat exchange system (chiller): available from Dhydra or can be customer supplied
- Internet connection: requires at least 1MBps
- Continuous monitoring by customer on-site via HMI

CERTIFICATIONS & APPROVALS

- Health Canada approved chemicals for CIP
- Electrical safety approved to CSA standards by LabTest Certification Inc.
- EU-GMP compliant RLTD System (in progress)
- ISO 9001 certified quality management system (in progress)
- Sanitation SOP
- Pass/Fail swab test

DIMENSIONS

Full system weight 6,863kg 15,130lb

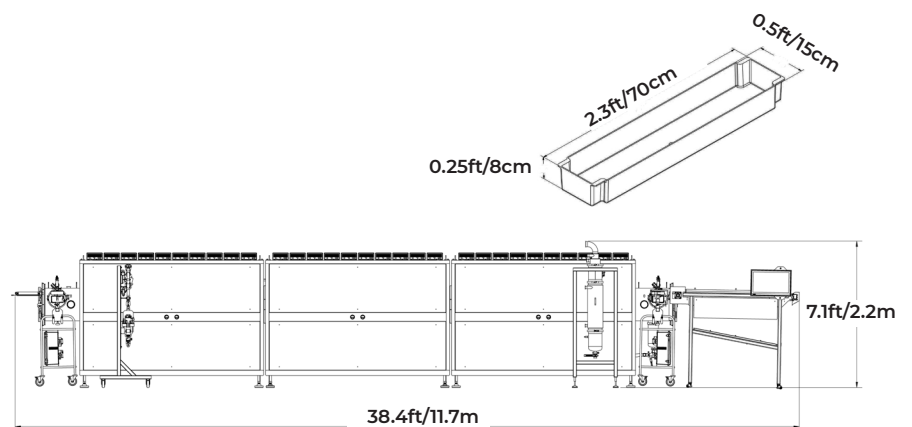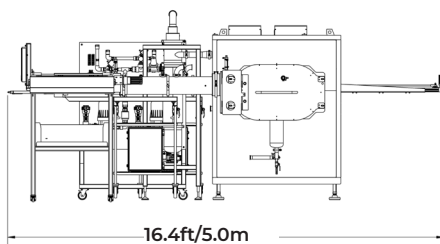

ROOM LAYOUT

